



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 11/28/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07J048

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1225 to 0.1229 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare (Handwritten signature)

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 17th day of December, 2007.

Linda L. DeSantis (Handwritten signature)
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Draegersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDWT 53-0363

Certification Date

Technician

Re-Certification Due Date

JAN. 21/2008

TE

JAN. 21/2009

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDONP2-229

Certification date:

02-12-08


Next Certification due:

02-12-09

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department



Drägersafety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

11/15/2006

SERIAL NUMBER:

ARWF-0382

Draeger Safety Diagnostics, Inc.
Durango, CO

LRD

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Serial No.: ARWF-0382
Location: WEST WINDSOR POLICE
Calibration File No.: 00415
Calib. Date: 05/30/2008
Calib. No.: 00010
Certification File No.: 00317
Cert. Date: 09/26/2007
Cert. No.: 00005
Linearity File No.: 00318
Lin. Date: 09/26/2007
Lin. No.: 00005
Solution File No.: 00412
Soln. Date: 05/20/2008
Soln. No.: 00050
Sequential File No.: 00415
File Date: 05/30/2008

Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDWJ S3-0363
Control Solution %: 0.100%
Expires: 02/22/2009
Solution Control Lot: 07B045
Bottle No.: 0074


Coordinator

Last Name: SNYDER
First Name: THOMAS
MI: J.

Signature: TPR. I Thomas J. Snyder #5792
Badge No.: 5792
Date: 05/30/2008

*Black Key Temperature Probe Serial# DDUNP2-229 SJJ

*Ertco-Hart Digital Temperature Measuring System Serial# 129881 SJJ

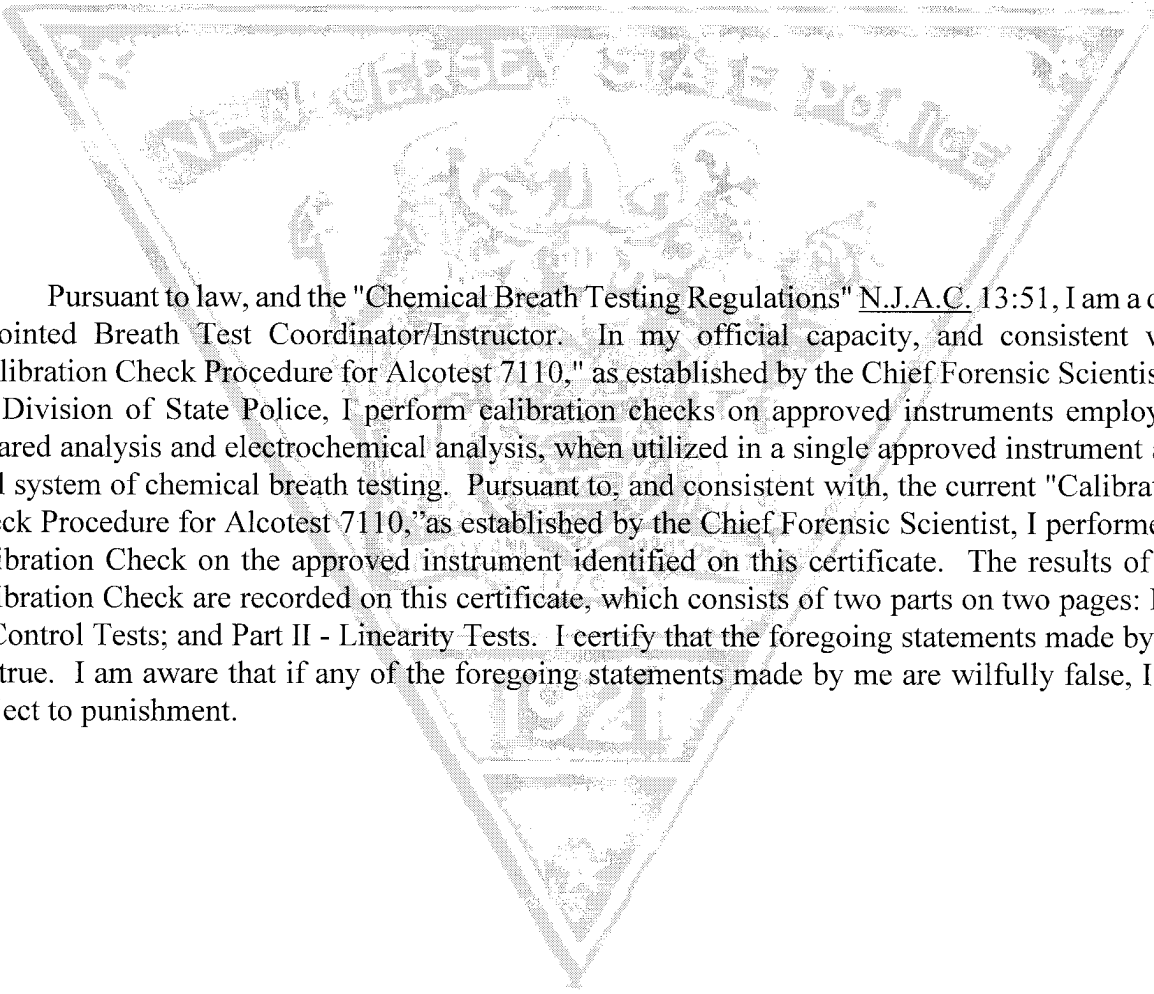

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0382
Location: WEST WINDSOR POLICE
Calibration File No.: 00415 Calib. Date: 05/30/2008 Calib. No.: 00010
Certification File No.: 00416 Cert. Date: 05/30/2008 Cert. No.: 00006
Linearity File No.: 00318 Lin. Date: 09/26/2007 Lin. No.: 00005
Solution File No.: 00412 Soln. Date: 05/20/2008 Soln. No.: 00050
Sequential File No.: 00416 File Date: 05/30/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0363
Control Solution %: 0.100% Expires: 02/22/2009
Solution Control Lot: 07B045 Bottle No.: 0074

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:30D		
Control 1 EC	0.100%	11:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	11:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31D		
Control 2 EC	0.099%	11:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:32D		
Control 3 EC	0.099%	11:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	11:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:34D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 05/30/2008

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0382
Location: WEST WINDSOR POLICE
Calibration File No.: 00415 Calib. Date: 05/30/2008 Calib. No.: 00010
Certification File No.: 00416 Cert. Date: 05/30/2008 Cert. No.: 00006
Linearity File No.: 00417 Lin. Date: 05/30/2008 Lin. No.: 00006
Solution File No.: 00412 Soln. Date: 05/20/2008 Soln. No.: 00050
Sequential File No.: 00417 File Date: 05/30/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0003
Control Solution %: 0.040% Expires: 01/26/2009
Solution Control Lot: 07A041 Bottle No.: 0511

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0184
Control Solution %: 0.080% Expires: 01/26/2009
Solution Control Lot: 07A042 Bottle No.: 0486

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0009
Control Solution %: 0.160% Expires: 01/26/2009
Solution Control Lot: 07A043 Bottle No.: 0096

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:55D		
Control 1 EC	0.041%	11:55D	33.8°C	*** TEST PASSED ***
Control 1 IR	0.040%	11:55D	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57D		
Control 2 EC	0.041%	11:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	11:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59D		
Control 3 EC	0.082%	11:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.081%	11:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:01D		
Control 4 EC	0.081%	12:01D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.081%	12:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:03D		
Control 5 EC	0.160%	12:03D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	12:03D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:05D		
Control 6 EC	0.160%	12:06D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.161%	12:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:07D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: THOMAS J. Snyder #5792

Badge No.: 5792

Date: 05/30/2008

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Thomas J. Snyder
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 17th DAY OF June TWO THOUSAND AND SIX

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 01/06)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Thomas J. Snyder
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF February TWO THOUSAND AND SIX

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 01/06)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Thomas J. Snyder
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breathalyzer A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 11th DAY OF Aug. TWO THOUSAND AND 00

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR	
1.	<u>11-14-04</u>	<u>ACTC</u>	<u>[Signature]</u>
2.	<u>5-5-03</u>	<u>OCPA</u>	<u>[Signature]</u>
3.	<u>4-4-05</u>	<u>ACTC</u>	<u>[Signature]</u>
4.			
5.			
6.			
7.			
8.			
9.			

SP-293B (Rev. 11/99)



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

STUART RABNER
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.


MANUFACTURER: Drager Safety, Inc. **ANALYSIS DATE:** 04/04/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07B045


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1222 to 0.1227 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is February 22, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.



 Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 30th day of April, 2007.

 Notary

Linda L. DeSantis
 My Commission
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





ION S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
West Trenton NJ 08628-0068
(609) 882-2000

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A041

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 29th day of March, 2007.

Notary



Linda L. DeSantis
My Commission
Expires Aug. 17, 2009

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

JON S. CORZINE
 Governor

STUART RABNER
 Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A042

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0965 to 0.0972 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare

Ajit R. Tungare
 Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 22nd day of March, 2007.

Linda L. DeSantis
 Notary

Linda L. DeSantis
 My Commission
 Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

STUART RABNER
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 03/06/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07A043

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1932 to 0.1938 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 26, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009

Ajit R. Tungare
Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 29th day of March, 2007.

Linda L. DeSantis
Notary



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



Calibrating Unit New Standard Solution Report


Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0382
Location: WEST WINDSOR POLICE
Calibration File No.: 00415 Calib. Date: 05/30/2008 Calib. No.: 00010
Certification File No.: 00416 Cert. Date: 05/30/2008 Cert. No.: 00006
Linearity File No.: 00417 Lin. Date: 05/30/2008 Lin. No.: 00006
Solution File No.: 00418 Soln. Date: 05/30/2008 Soln. No.: 00051
Sequential File No.: 00418 File Date: 05/30/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0363
Control Solution %: 0.100% Expires: 10/03/2009
Solution Control Lot: 07J048 Bottle No.: 0548

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:15D		
Control 1 EC	0.101%	13:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:16D		
Control 2 EC	0.100%	13:17D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17D		
Control 3 EC	0.100%	13:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWAP2-216 

Changed By:

Last Name: SNYDER


First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 05/30/2008



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST[®] CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDRK 53-0003

Certification Date


Technician

Re-Certification Due Date

02-13-08

[Signature]

02-13-09



Dräger safety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST[®] CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXDS3-0184

Certification Date

Technician

Re-Certification Due Date

02-13-08

[Signature]

02-13-09



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST[®] CU34
 Model: MARK IIA
 Other: _____

Serial Number:

DDSC 53-0009

Certification Date

02-13-08

Technician

Re-Certification Due Date

02-13-09

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWAP2-216

Certification date:

01-21-08

Next Certification due:

01-21-09

Probe Value

102

Draeger Safety Diagnostics, Inc.
Technical Service Department



Drägersafety

Ertco-Hart Digital Temperature Measuring System

REPORT OF CALIBRATION

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature verification Serial Number: HH41 301316 / HH41 303176 / MERCURY THERMOMETER

Digital Units Serial Number: A29881

Probe Serial Number: 590802

Certification Date: 02-12-2008

Next Certification Due: 02-12-2009

At 34.00 °C digital unit displays 34.06 °C

Draeger Safety Diagnostics, Inc. Technician: 