

Alcotest 7110 Calibration Record

Equipment

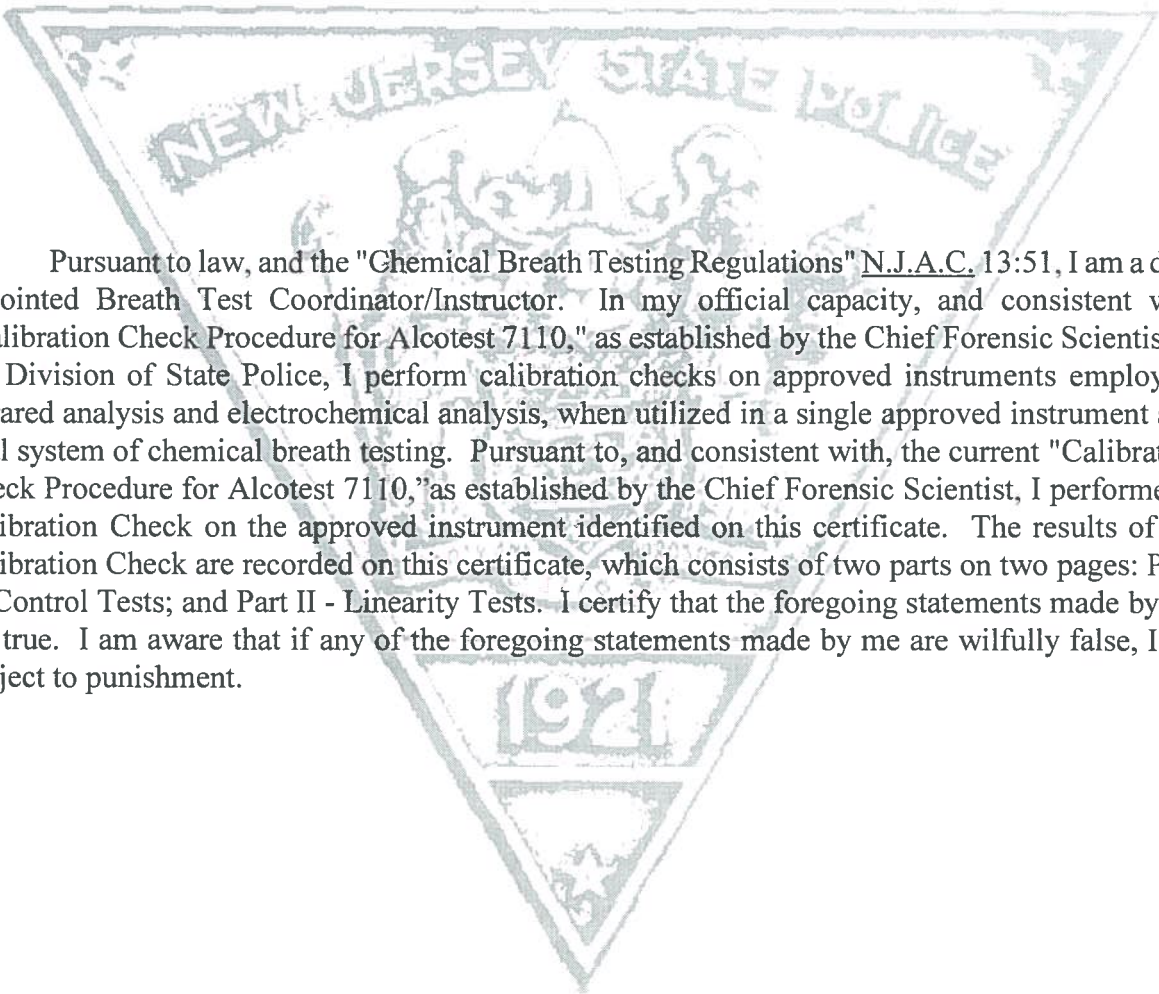
Alcotest 7110 MKIII-C
Serial No.: ARWF-0382
Location: WEST WINDSOR POLICE
Calibration File No.: 01222
Calib. Date: 06/10/2015
Calib. No.: 00034
Certification File No.: 01170
Cert. Date: 01/08/2015
Cert. No.: 00021
Linearity File No.: 01171
Lin. Date: 01/08/2015
Lin. No.: 00021
Solution File No.: 01216
Soln. Date: 05/18/2015
Soln. No.: 00175
Sequential File No.: 01222
File Date: 06/10/2015

Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDWJ S3-0364
Control Solution %: 0.100%
Expires: 09/23/2015
Solution Control Lot: 131123
Bottle No.: 0100

Coordinator

Last Name: GONCALVES
First Name: MICHELLE
MI: L
Signature: Sgt Michelle Goncalves #6040
Badge No.: 6040
Date: 06/10/2015

*Black Key Temperature Probe Serial.....# DDUNP2-231 (MA)
*Digital NIST Temperature Measuring System Serial.....# 130602271 (MA)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0382
Location: WEST WINDSOR POLICE
Calibration File No.: 01222 Calib. Date: 06/10/2015 Calib. No.: 00034
Certification File No.: 01223 Cert. Date: 06/10/2015 Cert. No.: 00022
Linearity File No.: 01171 Lin. Date: 01/08/2015 Lin. No.: 00021
Solution File No.: 01216 Soln. Date: 05/18/2015 Soln. No.: 00175
Sequential File No.: 01223 File Date: 06/10/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWJ S3-0364
Control Solution %: 0.100% Expires: 09/23/2015
Solution Control Lot: 13I123 Bottle No.: 0100

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:12D		
Control 1 EC	0.099%	10:13D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:13D		
Control 2 EC	0.099%	10:14D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:15D		
Control 3 EC	0.099%	10:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:16D		

All tests within acceptable tolerance.

Coordinator

Last Name: GONCALVES First Name: MICHELLE MI: L

Signature: Sgt. Michelle Goncalves #6040 Badge No.: 6040
Date: 06/10/2015

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARWF-0382
Location: WEST WINDSOR POLICE
Calibration File No.: 01222 Calib. Date: 06/10/2015 Calib. No.: 00034
Certification File No.: 01223 Cert. Date: 06/10/2015 Cert. No.: 00022
Linearity File No.: 01224 Lin. Date: 06/10/2015 Lin. No.: 00022
Solution File No.: 01216 Soln. Date: 05/18/2015 Soln. No.: 00175
Sequential File No.: 01224 File Date: 06/10/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0003
Control Solution %: 0.040% Expires: 09/13/2015
Solution Control Lot: 13I120 Bottle No.: 0445

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAE-0022
Control Solution %: 0.080% Expires: 09/16/2015
Solution Control Lot: 13I121 Bottle No.: 1289

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDCN-0052
Control Solution %: 0.160% Expires: 08/05/2016
Solution Control Lot: 14H131 Bottle No.: 1091

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:39D		
Control 1 EC	0.042%	10:39D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	10:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41D		
Control 2 EC	0.041%	10:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	10:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43D		
Control 3 EC	0.081%	10:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.081%	10:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:45D		
Control 4 EC	0.081%	10:46D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	10:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47D		
Control 5 EC	0.161%	10:48D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	10:48D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:50D		
Control 6 EC	0.159%	10:50D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.160%	10:50D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:52D		

All tests within acceptable tolerance.

Coordinator

Last Name: GONCALVES

First Name: MICHELLE

MI: L

Signature: 

Badge No.: 6040

Date: 06/10/2015



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDWJ33-0364

Certification Date

Technician

Re-Certification Due Date

4-30-15

BC

4-30-16

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe, within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDWA Pa-215

4-24-15

4-24-16

Probe Value

107

Draeger Safety Diagnostics, Inc.
Technical Service Department

BC



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 5/6/2015

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 15D138

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 13, 2017.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 7th day of May, 2015.

Notary
MARY ELIZABETH MCLAUGHLIN
 ID # 2062190
 NOTARY PUBLIC
 STATE OF NEW JERSEY
 My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
Governor
 KIM GUADAGNO
Lt. Governor

JOHN J. HOFFMAN
Acting Attorney General
 COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 9/11/2014

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 14H132

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1211 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 22, 2016.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15th day of September, 2014.

Notary

LINDA L DESANTIS
 ID # 2228589
 NOTARY PUBLIC
 STATE OF NEW JERSEY
 My Commission Expires August 17, 2019



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





CERTIFICATE

This is to certify that


Michelle Goncalves

has successfully completed the two day Draeger Safety Diagnostics, Inc. Alcohol Coordinator Training Course on the New Jersey specific Alcotest® 7110 MKIII-C and is hereby certified as a qualified

**Operator Trainer and
Maintenance Technician**

Completion of this course qualifies this individual to train and certify Operators in the proper use and operation as well as perform Preventive Maintenance on the New Jersey specific Alcotest® 7110 MKIII-C.

Date: March 14, 2012


Instructor: Hansueli Ryser

Dräger



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-5427014

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087
Instrument Identification:

Model: 61220-601 S/N: 130802271 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-17B	A45240		
Thermistor Module	A17118	2/13/14	1000332071
Temperature Probe	128	2/20/14	6-B4829-30-1
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A17118	2/13/14	1000332071
Temperature Probe	3039	2/20/14	6-B4829-1-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Module	A27129	11/08/13	1000327281
Temperature Probe	5202	11/30/14	15-B15PW-1-1
Temperature Calibration Bath TC-273	B16388		
Digital Thermometer	B18815	8/12/14	1000341987
PRT Temperature Probe	02022	8/14/15	83812004

Certificate Information:

Technician: 68 Procedure: CAL-08 Cal Date: 10/08/13 Cal Due: 10/08/15
Test Conditions: 24.0°C 37.0 %RH 1017 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.001	0.000	Y	-0.051	0.049	0.013	3.8:1
°C		N.A.		25.001	25.000	Y	24.951	25.051	0.023	2.2:1
°C		N.A.		50.003	50.001	Y	49.953	50.053	0.014	3.6:1
°C		N.A.		100.001	99.994	Y	99.951	100.051	0.018	2.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the items calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal-Standard's Reading; As Left-Instrument's Reading; In Tol-In Tolerance; Min/Max-Acceptance Range; ±U-Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judon
Aaron Judon, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01305-2005-AQ-HOU-RVA
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

DEPARTMENT OF
Traffic and Public Safety
It is to be recalled that

Michelle Goncalves
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT COURSE IN THE STATE OF NEW JERSEY IN ACCORDANCE TO CHAPTER 1407
TITLE 17, PART 26 OF THE COMPANION STATUTES
A LICENSED INSTRUCTOR IN THE COURSE OF INSTRUCTION
COURSE NUMBER: 7118 MOIU-C

THIS COURSE IS IN EFFECT

December

[Signature]
INSTRUCTOR
NEW JERSEY STATE POLICE

[Signature]
ATTEST: CLERK
NEW JERSEY STATE POLICE

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 12-3-13	GC PA	Kim Lero
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2018 (Rev. 05/10)

DEPARTMENT OF
Traffic and Public Safety
It is to be recalled that

Michelle Goncalves
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT COURSE IN THE STATE OF NEW JERSEY IN ACCORDANCE TO CHAPTER 1407
TITLE 17, PART 26 OF THE COMPANION STATUTES
A LICENSED INSTRUCTOR IN THE COURSE OF INSTRUCTION
COURSE NUMBER: 7118 MOIU-C

THIS COURSE IS IN EFFECT

March

[Signature]
INSTRUCTOR
NEW JERSEY STATE POLICE

[Signature]
ATTEST: CLERK
NEW JERSEY STATE POLICE

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2018 (Rev. 05/10)



CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lieutenant Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF CRIMINAL JUSTICE
PO BOX 083
TRENTON, NJ 08625-0083
TELEPHONE: (609) 984-6300

JEFFREY S. CHIESA
Attorney General

STEPHEN J. TAYLOR
Director

March 23, 2012

Col. Joseph R. Fuentes, Superintendent
Division of State Police
Division Headquarters
P.O. Box 7068
West Trenton, New Jersey 08628

Re: Breath Test Coordinator/Instructor, Certification -
Detective I Michelle L. Goncalves #6040

Dear Col. Fuentes:

Pursuant to the provisions of *N.J.A.C.* 13:51-2.1 (b) and (c), as adopted and promulgated under the provisions of *N.J.S.A.* 39:4-50.3, 39:3-10.25 and 12:7-56, I hereby approve Detective I Michelle L. Goncalves #6040, as a duly certified Breath Test Coordinator/Instructor. This approval is effective immediately.

Very truly yours,

Jeffrey S. Chiesa
Attorney General

- c. Detective I Michelle L. Goncalves, Alcohol/Drug Test Unit, Division of State Police
DSFC Patrick Guilfooy, Unit Head, Alcohol/Drug Test Unit, Division of State Police





Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDMKS3-0003

Certification Date

Technician

Re-Certification Due Date

9-19-14

BC

9-19-15



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDCN-0052

Certification Date

Technician

Re-Certification Due Date

9-22-14

BC

9-22-15



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDAE-0022

Certification Date

8-28-14

Technician

BC

Re-Certification Due Date

8-28-15

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe, within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDUNP2-231

Certification date:

9-19-14

Next Certification due:

9-19-15

Probe Value

107

Dräger Safety Diagnostics, Inc.
Technical Service Department

BC



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/25/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 13I120

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0489 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 13, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Ajaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of October, 2013.

Linda L. Demaris
 Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/31/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 13I121

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0959 to 0.0971 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 16, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 1st day of November, 2013.

Mary E. McLaughlin
 Notary

MARY ELIZABETH MCLAUGHLIN
 NOTARY PUBLIC OF NEW JERSEY
 MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.


ANALYSIS DATE: 8/14/2014

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 14H131


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1925 to 0.1944 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 5, 2016.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Ali M. Alaoui, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 14th day of August, 2014.


 Notary
MARY ELIZABETH MCLAUGHLIN
 ID # 2052190
 NOTARY PUBLIC
 STATE OF NEW JERSEY
 My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/24/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 131123

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1186 to 0.1192 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 23, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20th day of October, 2013.

Linda L. Alaouie
 Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable

