

# Alcotest 7110 Calibration Record

## Equipment

Location: Alcotest 7110 MKIII-C  
WEST WINDSOR POLICE  
Calibration File No.: 01751  
Certification File No.: 01725  
Linearity File No.: 01726  
Solution File No.: 01750  
Sequential File No.: 01751

Calib. Date: 02/24/2022  
Cert. Date: 09/21/2021  
Lin. Date: 09/21/2021  
Soln. Date: 02/06/2022  
File Date: 02/24/2022

Serial No.: ARWF-0382  
Calib. No.: 00056  
Cert. No.: 00039  
Lin. No.: 00038  
Soln. No.: 00298

Calibrating Unit: WET  
Control Solution %: 0.100%  
Solution Control Lot: 20220

Model No.: CU-34

Serial No.: DDWJ S3-0364  
Expires: 05/06/2022  
Bottle No.: 1150

## Coordinator

Last Name: GUARCELLO

First Name: COREY


MI: R.

Signature:  # 7035

Badge No.: 7035

Date: 02/24/2022

\*Black Key Temperature Probe Serial.....# DDXK P2-398 (CG)  
\*Digital NIST Temperature Measuring System Serial.....# 210 216801 (CG)

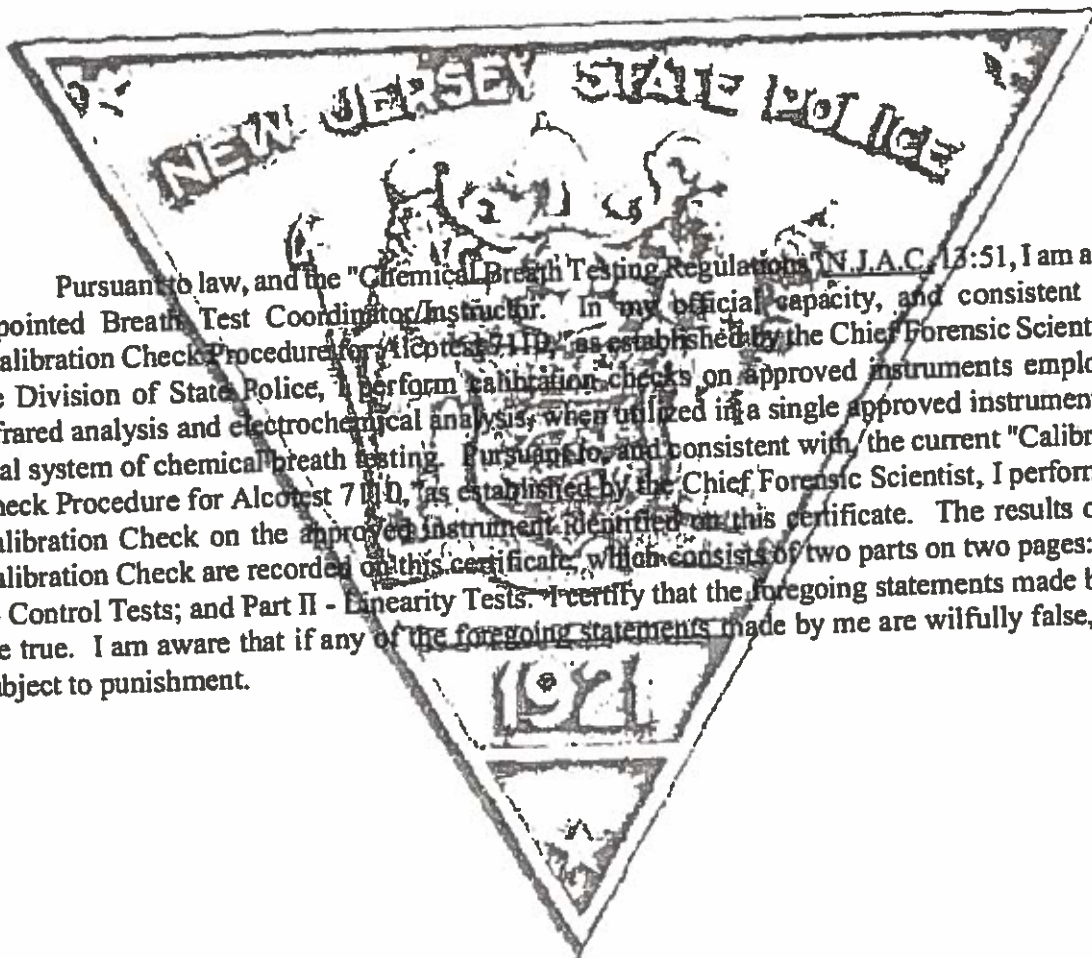

Pursuant to law, and the "Chemical Breath Testing Regulations N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.