

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWF-0382
Location:	WEST WINDSOR POLICE	
Calibration File No.:	01118	Calib. Date: 07/09/2014
Certification File No.:	01119	Calib. No.: 00032
Linearity File No.:	01120	Cert. Date: 07/09/2014
Solution File No.:	01167	Cert. No.: 00020
Sequential File No.:	01167	Lin. Date: 07/09/2014
		Lin. No.: 00020
		Soln. Date: 12/25/2014
		Soln. No.: 00166
		File Date: 12/25/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0363
Solution Control Lot:	14H132	Expires: 08/22/2016
		Bottle No.: 1253

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:29S		
Control 1 EC	0.097%	11:30S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:30S		
Control 2 EC	0.096%	11:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:32S		
Control 3 EC	0.096%	11:32S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	11:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: BAL

First Name: FRANK

MI: N

Signature:

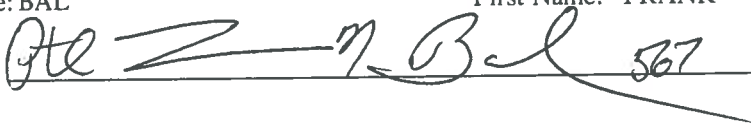

Badge No.: 567

Date: 12/25/2014