

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWF-0382
Location:	WEST WINDSOR POLICE	
Calibration File No.:	01169	Calib. Date: 01/08/2015
Certification File No.:	01170	Calib. No.: 00033
Linearity File No.:	01171	Cert. Date: 01/08/2015
Solution File No.:	01197	Cert. No.: 00021
Sequential File No.:	01197	Lin. Date: 01/08/2015
		Lin. No.: 00021
		Soln. Date: 03/11/2015
		Soln. No.: 00172
		File Date: 03/11/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0363
Solution Control Lot:	14H132	Expires: 08/22/2016
		Bottle No.: 1273

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:28S		
Control 1 EC	0.100%	06:29S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:30S		
Control 2 EC	0.097%	06:30S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	06:30S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:31S		
Control 3 EC	0.099%	06:32S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	06:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: TARR

First Name: MARYLOUISE

MI: -

Signature: _____

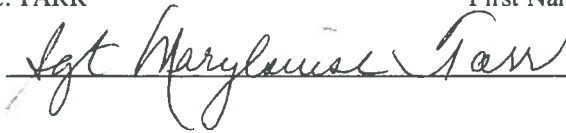

Badge No.: 431

Date: 03/11/2015