

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWF-0382
Location:	WEST WINDSOR POLICE	
Calibration File No.:	01074	Calib. Date: 02/06/2014
Certification File No.:	01075	Calib. No.: 00031
Linearity File No.:	01076	Cert. Date: 02/06/2014
Solution File No.:	01115	Cert. No.: 00019
Sequential File No.:	01115	Lin. Date: 02/06/2014
		Lin. No.: 00019
		Soln. Date: 06/27/2014
		Soln. No.: 00157
		File Date: 06/27/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDWJ S3-0364
Solution Control Lot:	13G115	Expires: 07/18/2015
		Bottle No.: 0008

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:46D		
Control 1 EC	0.099%	10:47D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:48D		
Control 2 EC	0.098%	10:48D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:49D		
Control 3 EC	0.098%	10:50D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:50D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: TARR

First Name: MARYLOUISE

MI: -

Signature: \_\_\_\_\_

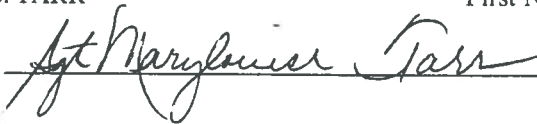

Badge No.: 431

Date: 06/27/2014