

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWF-0382
Location:	WEST WINDSOR POLICE		
Calibration File No.:	00984	Calib. Date:	02/26/2013
Certification File No.:	00985	Cert. No.:	00029
Linearity File No.:	00986	Cert. Date:	02/26/2013
Solution File No.:	01028	Lin. Date:	02/26/2013
Sequential File No.:	01028	Lin. No.:	00017
		Soln. Date:	07/29/2013
		Soln. No.:	00140
		File Date:	07/29/2013
Calibrating Unit:	WET	Model No.:	4
Control Solution %:	0.100%	Serial No.:	DDWJ S3-0363
Solution Control Lot:	12L109	Expires:	12/26/2014
		Bottle No.:	0115

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:06D		
Control 1 EC	0.100%	16:06D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:07D		
Control 2 EC	0.098%	16:07D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:08D		
Control 3 EC	0.099%	16:09D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:09D		

All tests within acceptable tolerance.

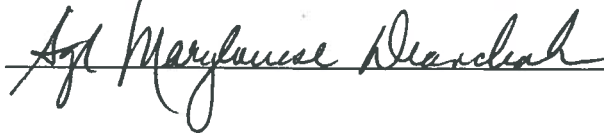
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DRANCHAK

First Name: MARYLOUISE

MI: -

Signature: 

Badge No.: 431

Date: 07/29/2013

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWF-0382
Location:	WEST WINDSOR POLICE		
Calibration File No.:	00984	Calib. Date:	02/26/2013
Certification File No.:	00985	Cert. Date:	02/26/2013
Linearity File No.:	00986	Lin. Date:	02/26/2013
Solution File No.:	01027	Soln. Date:	07/29/2013
Sequential File No.:	01027	File Date:	07/29/2013
Calibrating Unit:	WET	Model No.:	4
Control Solution %:	0.100%	Serial No.:	DDWJ S3-0363
Solution Control Lot:	12L109	Expires:	12/26/2014
		Bottle No.:	0120

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:28D		
Control 1 EC	-.---%	11:29D	34.0°C	CTRL GAS SUPPLY
Control 1 IR	-.---%	11:29D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: DRANCHAK

First Name: MARYLOUISE

MI: -

Signature:



Badge No.: 431

Date: 07/29/2013